

#### Please cite the Published Version

Reeves, ND <sup>(i)</sup>, Culmer, P, Venkatraman, P <sup>(i)</sup>, Turnbul, RP, Bradbury, K, Corser, J, Orlando, G <sup>(i)</sup> and Yoldi, I (2024) 'Socksess' - Smart Sensing Socks for Monitoring Diabetic Feet and Preventing Ulceration. In: EPSRC digital health policy event at London Institute of Healthcare Engineering [LIHE], 17 October 2024, London Institute for Healthcare Engineering, London, UK. (Unpublished)

Version: Published Version

Downloaded from: https://e-space.mmu.ac.uk/636673/

Usage rights: C In Copyright

#### Enquiries:

If you have questions about this document, contact openresearch@mmu.ac.uk. Please include the URL of the record in e-space. If you believe that your, or a third party's rights have been compromised through this document please see our Take Down policy (available from https://www.mmu.ac.uk/library/using-the-library/policies-and-guidelines)











# 'Socksess' - Smart Sensing Socks for Monitoring Diabetic Feet and Preventing Ulceration (EP/X001059/1)

Neil D. Reeves<sup>1</sup>, Peter R. Culmer<sup>2</sup>, Rory P. Turnbull<sup>2</sup>, Katherine Bradbury<sup>3</sup>, Jenny Corser<sup>3</sup>, Prabhuraj D. Venkatraman<sup>4</sup>, Giorgio Orlando<sup>4</sup>, Irantzu Yoldi<sup>5</sup>.

# **Project Vision**

Diabetic neuropathy (nerve damage) causes a loss of sensation in the foot, which is one of the major risk factors for developing diabetic foot ulcers. This loss of foot sensation removes people's ability to 'naturally' self-regulate their foot pressures and over time this causes tissue breakdown and ulceration, with subsequent limb amputation, or death as ultimate consequences, with NHS costs >£1billion annually. This presents an opportunity for a health technology solution to support and empower people with their foot health.

Current solutions include smart insole systems constrained by footwear requirements and presenting barriers to adoption and adherence. A crucial engineering-based innovation gap is that no system is capable of measuring shear stress, increasingly recognised as an important contributor to diabetic foot ulcer development.

The 'Socksess' project vision is to develop 'smart-sensing socks' addressing innovation gaps and providing a novel solution for daily monitoring and prevention of diabetic foot ulcers.

## **Project Aims**

- The project **aim** is to co-design, develop and test an ambitious new healthcare 2. monitoring technology focused on preventing diabetic foot ulcers through
- Develop and evaluate candidate sensor technologies for measurement of shear stress and to integrate these within stretchable sock fabric with electrical connectivity.

#### 'reconnecting people with their feet'.

Specific project objectives are:

- To understand the needs and preferences of people with diabetes, their carers and clinicians, to co-design a smart-sensing sock.
- Test and validate the smart-sensing socks in a cohort of people at high-risk for 3. diabetic foot ulceration.
- 4. Co-design with relevant stakeholders a highly accessible feedback system to alert the user when they are at risk of foot ulceration.

# **Key Outcomes and Results**

### **Co-Designing the Technology with Stakeholders**

A qualitative study was undertaken with key stakeholders including 20 people with diabetic neuropathy (n=16 with history of diabetic foot ulcers), carers (n=2) and podiatrists (*n*=6). Three main themes were generated.

- 1. Patient buy-in: challenged by lack of awareness of risk, and potentially addressed though using the device to collect and record evidence to enhance clinical messaging.
- **Effective engagement:** challenged by difficulties accepting and actioning 2. information, requiring simple, specific and supportive instructions in line with podiatrist advice.
- **Sustained use:** challenged by difficulties coping, with the possibility to gain 3. control with an early warning system.

### **Design & Development of Socks Material**

We used an industry-grade socks knitting machine (with integral toe closure) at sensor signals to be passed to the socks welt area Manchester Fashion Institute, to fabricate our custom-designed socks.

### **Shear Sensor Design and Development**

Manufacture: Sensors were produced using a Workbee CNC coupled to a Nordson dispensing system, allowing for the 3D printing of our sensors (Fig. 3).

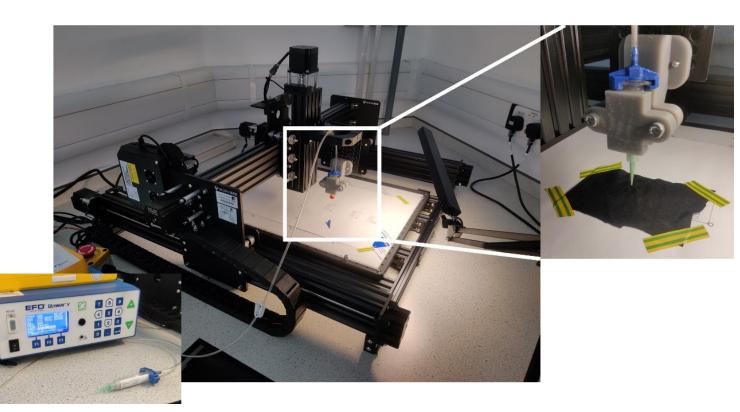



Figure 3. System used for 3D printing the shear sensors.

**Parametric Study:** After extensive investigation of potential materials, a silver adhesive by Dycotec was Parametric testing selected. was initially undertaken on a Lycra substrate before integration with sock material. This approach enabled development prior to the additional challenges introduced with 3D printing onto knitted structures (Fig. 4).

**Sensor Integration:** conductive yarns allowed for


We explored novel sock designs, the composition of sock material, knit structure, yarn type, and fibre composition to optimise performance and incorporation of sensing elements within the sock. The development process has been guided by stakeholder input, qualitative research, and garment design factors (Fig. 1).


Socks were made using 78 dtex recycled nylon yarns, 44 dtex Lycra/nylon blended yarns, 30/1 Ne combed cotton yarns and elastic filament.

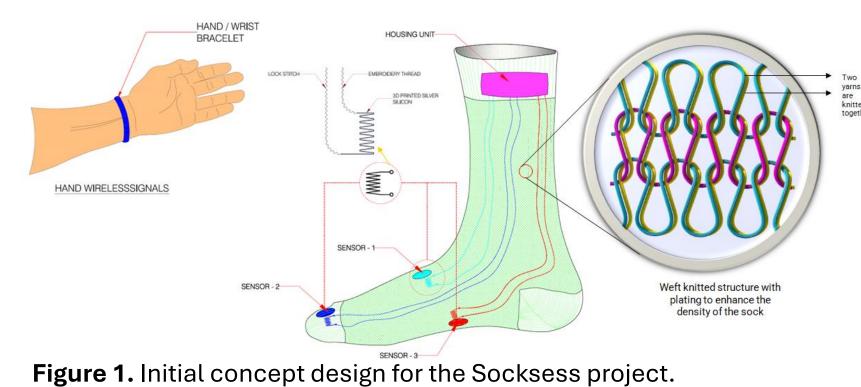

We have developed socks with embroidered conductive yarns to connect with flexible resistancebased strain sensors. Following extensive development work, we have refined our shortlist to two types of socks (Fig. 2).

in a flexible manner. Sensor signals were collected through an Arduino based microcontroller in MAX31865 combination with a resistance temperature detector amplifier. Traditionally the chip is used to measure temperature, however, we have applied it as a high-resolution method of measuring resistance. Additionally, the 4-wire thermocouple method enabled us to account for the resistance induced by the conductive yarns. Custom connectors were produced to form an interface between sock and electronic components (Fig. 5). A custom PCB was designed to house two of the MAX31865 breakouts by Adafruit supporting the placement of two sensors on the sock (Fig. 5).

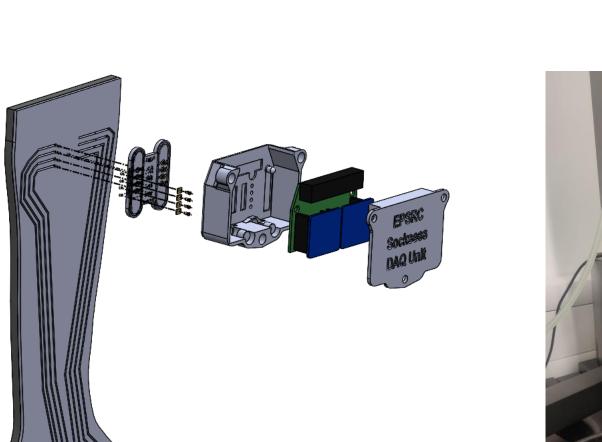

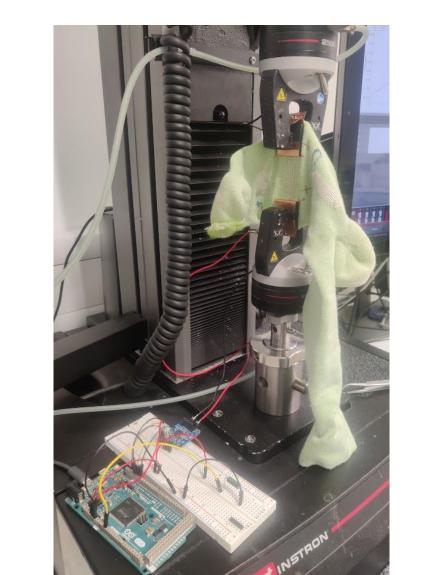

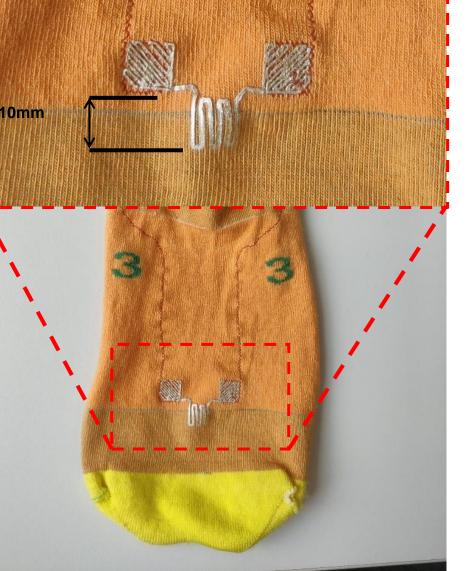


Figure 4. Silver adhesive sensors 3Dprinted onto the sock material, connecting up with the embroidered conductive fibres.


#### **Sensor Assessment:**

samples were loaded (quasistatic and cyclic) on an Instron (Fig. 6) to determine performance strain gauge and inform final design based on parametric results. The knitted structure improved performance by acting as a new composite structure. Sensor reinforcement with a silicone coating allowed us to tune responsiveness while also protecting from the local environment.

The conductive thread embroidery pattern can be seen in the supplementary

material (scan QR code below).



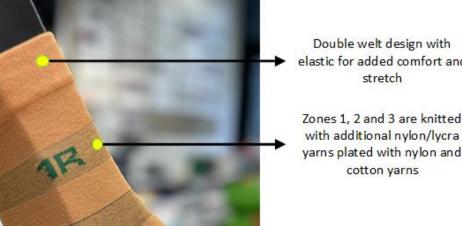




Figure 5. Exploded diagram showing sensor placement, embroidered conductive yarn paths and custom electronic connector components.


Figure 6. Intron machine and sensor testing environment.

# **Next Steps**



information

We are embarking on human user trials to test the smart-sensing socks in people with diabetic neuropathy (Fig. 7).

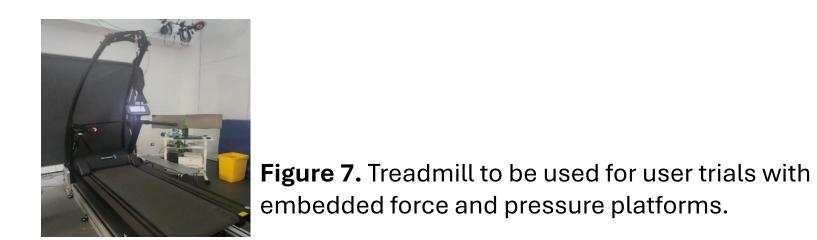

The team are now planning to further develop the technology by refining key features, advancing TRL and developing a route towards commercialisation. Funding routes to support this are being explored.

Further technology development: This project has produced major innovations, driven by co-production and novel research.